Publication No. 7H2718
28NOV07
Supersedes 7H2718
07NOV07

CARRIER UNPACKING INSTRUCTIONS

for the

Kodak DirectView CLASSIC/ELITE CR SYSTEMS

Service Code: 5258, 5259

Important

When performing the procedures outlined in this publication, personnel must always employ safe work practices and wear the appropriate personal protective equipment (e.g. safety eye wear) in accordance with their Company's Safety and Health Policies and Procedures

Carestream HEALTH

© CARESTREAM HEALTH, INC. 2007

PLEASE NOTE The information contained herein is based on the experience and knowledge relating to the subject matter gained by Carestream Health, Inc. prior to publication.

No patent license is granted by this information.

Carestream Health, Inc. reserves the right to change this information without notice, and makes no warranty, express or implied, with respect to this information. Carestream Health shall not be liable for any loss or damage, including consequential or special damages, resulting from any use of this information, even if loss or damage is caused by Carestream Health's negligence or other fault.

This equipment includes parts and assemblies sensitive to damage from electrostatic discharge. Use caution to prevent damage during all service procedures.

Table of Contents

Description	Page
Unpacking the Equipment	3

Unpacking the Equipment

Caution

When performing the procedures outlined in this publication, personnel must always employ safe work practices and wear the appropriate personal protective equipment (e.g. safety eye wear) in accordance with their Company's Safety and Health Policies and Procedures

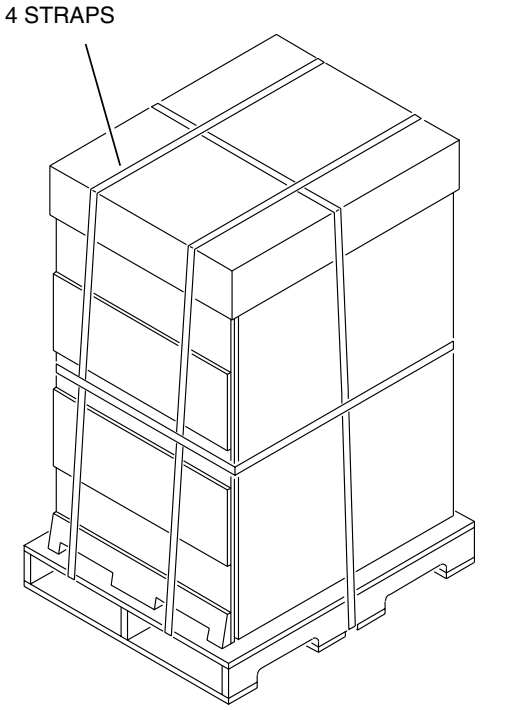

H219_3012GCA
H219_3012GC

[1] Check the SHOCK WATCH on the side of the carton.

[2] Is the SHOCK WATCH red?

Yes	No
Stop the installation procedure and call the Technical Support Center (TSC).	Continue with Step 3.

[3] Record any problems that occur during this installation. Include this information in the "OUT OF BOX SURVEY" you provide to the customer.

Caution

Be careful when you cut the STRAPS. The STRAPS are tight.

[4] Cut the 4 STRAPS.

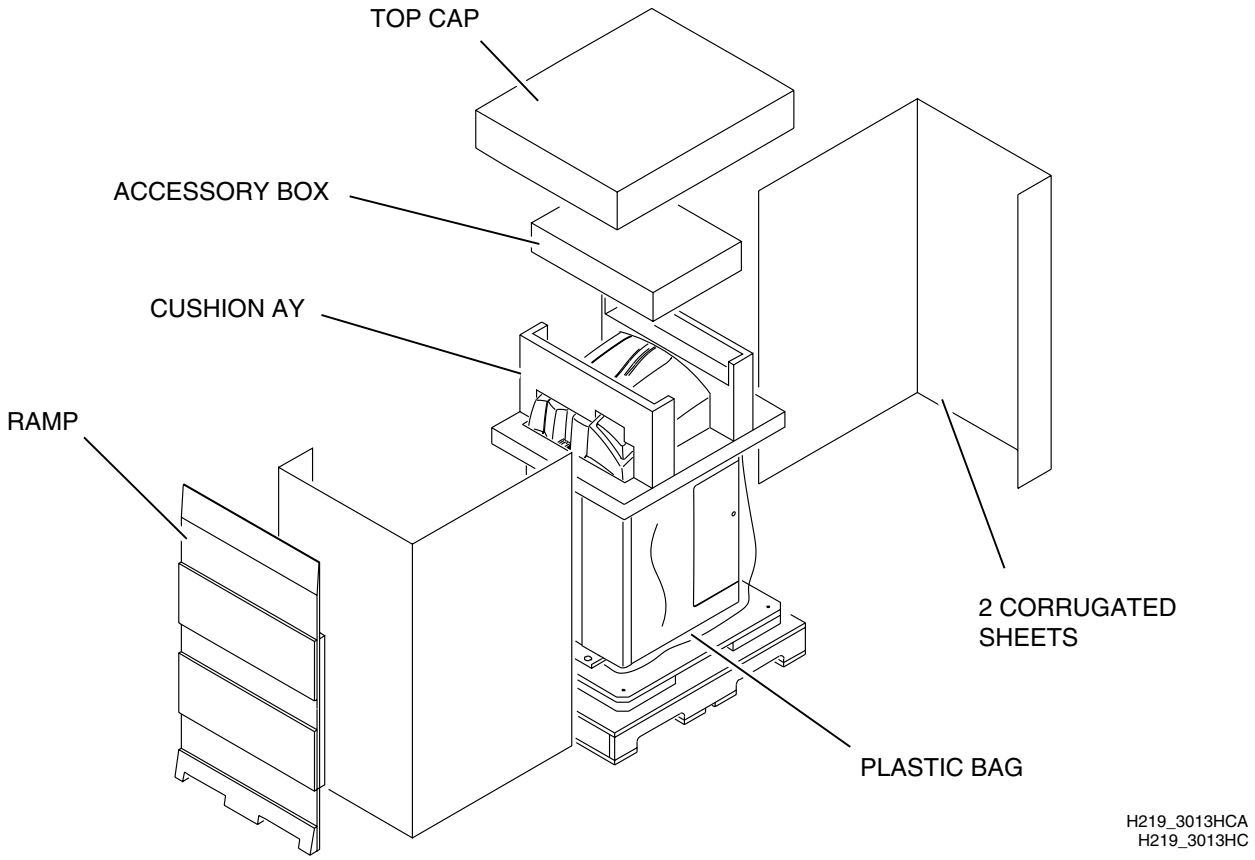

Caution

The RAMP is held by the TOP CAP. Be careful when you remove the TOP CAP. The RAMP might fall.

[5] Remove:

- TOP CAP
- RAMP
- 2 CORRUGATED SHEETS
- ACCESSORY BOX
- CUSHION AY
- PLASTIC BAG

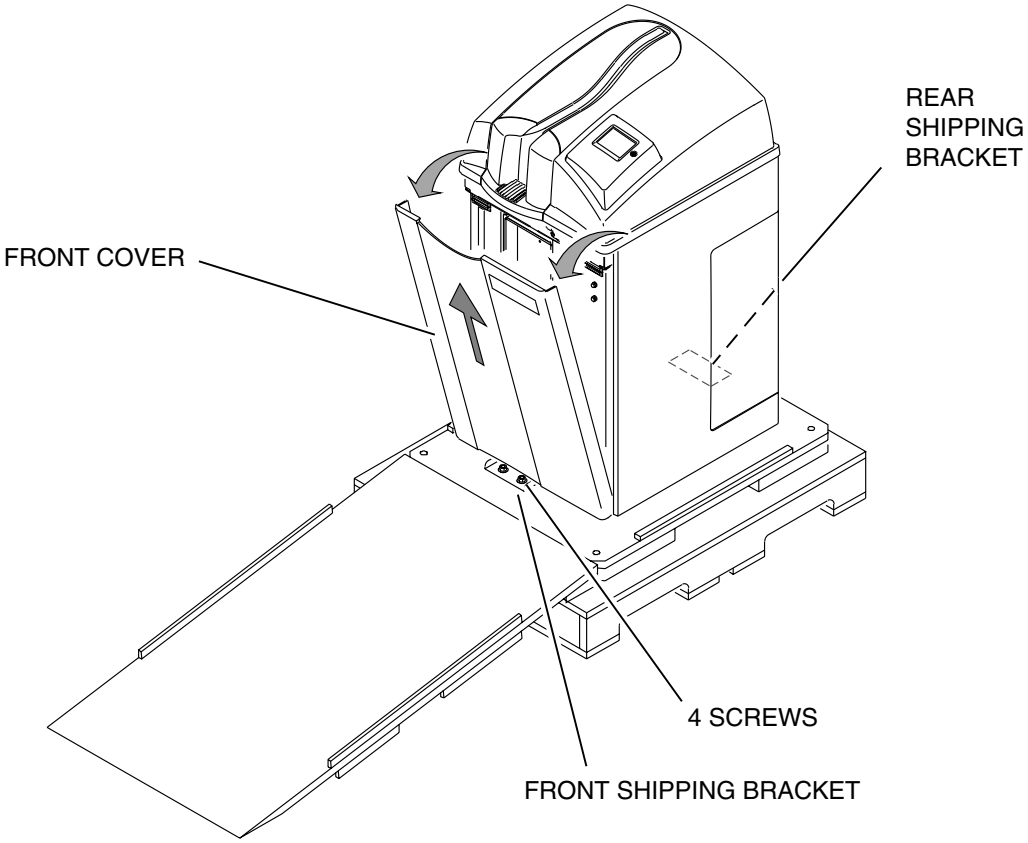

H219_3042HCA
H219_3042HC

[6] Pull and lift to remove the FRONT COVER.

Important

Keep the 2 SHIPPING BRACKETS.

[7] Remove and keep:

- 4 SCREWS
- FRONT SHIPPING BRACKET
- 4 SCREWS
- REAR SHIPPING BRACKET

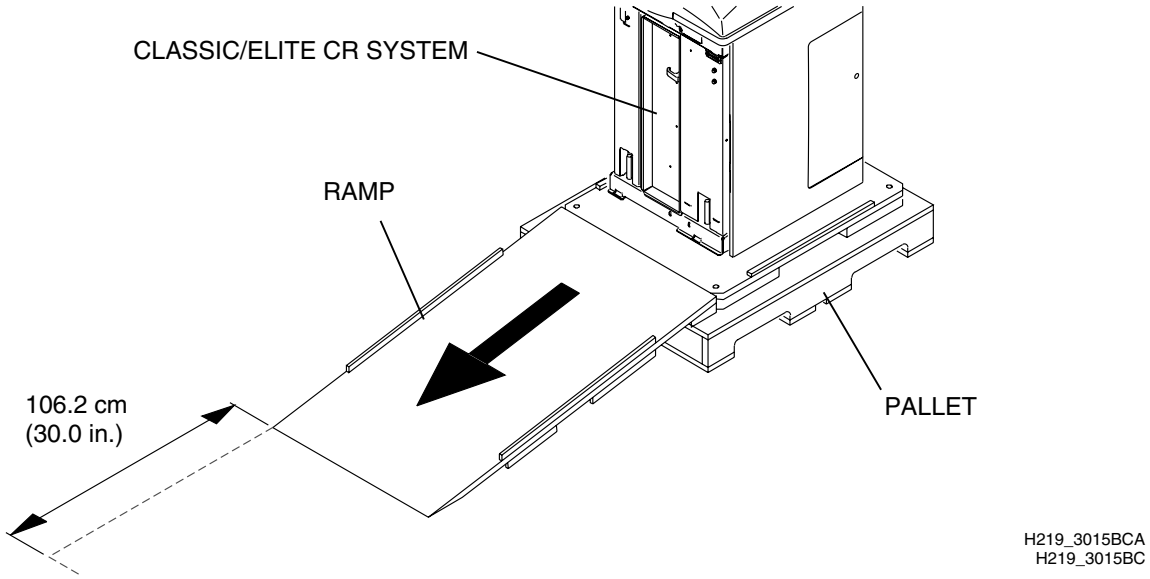

H219_3015BCA
H219_3015BC

Caution

You must have a minimum of 106.2 cm (30.0 in.) of clearance at the end of the RAMP to move the CLASSIC/ELITE CR SYSTEM.

[8] Fasten the RAMP to the PALLET.

Caution

The weight is 140.9 kg (310 lb). Be careful when you move the system down the RAMP.

[9] Carefully move the system down the RAMP.

[10] Install the FRONT COVER.

[11] Remove any other ACCESSORY BOXES from PALLETS and place next to the CLASSIC/ELITE CR SYSTEM.

Publication History

Publication Date	Publication No.	ECO No.	Changed Pages	File Name	Notes
07NOV07	7H2718	----	All	7h2718.fm	New Publication
28NOV07	7H2718	----	1	7h2718.fm	Added Caution.

DirectView is a trademark of Carestream Health.
Kodak is a trademark of Kodak used under license.

Printed in U.S.A. • 7h2718.fm

Carestream Health, Inc.
150 Verona Street
Rochester, NY 14608